


```

=====
Acq. Operator   : KKT                               Seq. Line :   11
Acq. Instrument : Instrument 1                       Location  : Vial 8
Injection Date  : 9/7/2020 5:14:41 PM                Inj       :    1
                                                    Inj Volume: 10.0 µl

Acq. Method     : Z:\LC\PODPIWEK ZAW_ALKOHOLU 2020-09-07 12-15-23\WZORCE_K_FERMENT.M
Last changed    : 9/7/2020 1:05:49 PM by KKT
                  (modified after loading)

Analysis Method : C:\CHEM32\1\METHODS\WZORCE_K_FERMENT.M
Last changed    : 9/8/2020 11:56:12 AM by KKT
                  (modified after loading)

Additional Info : Peak(s) manually integrated
  
```

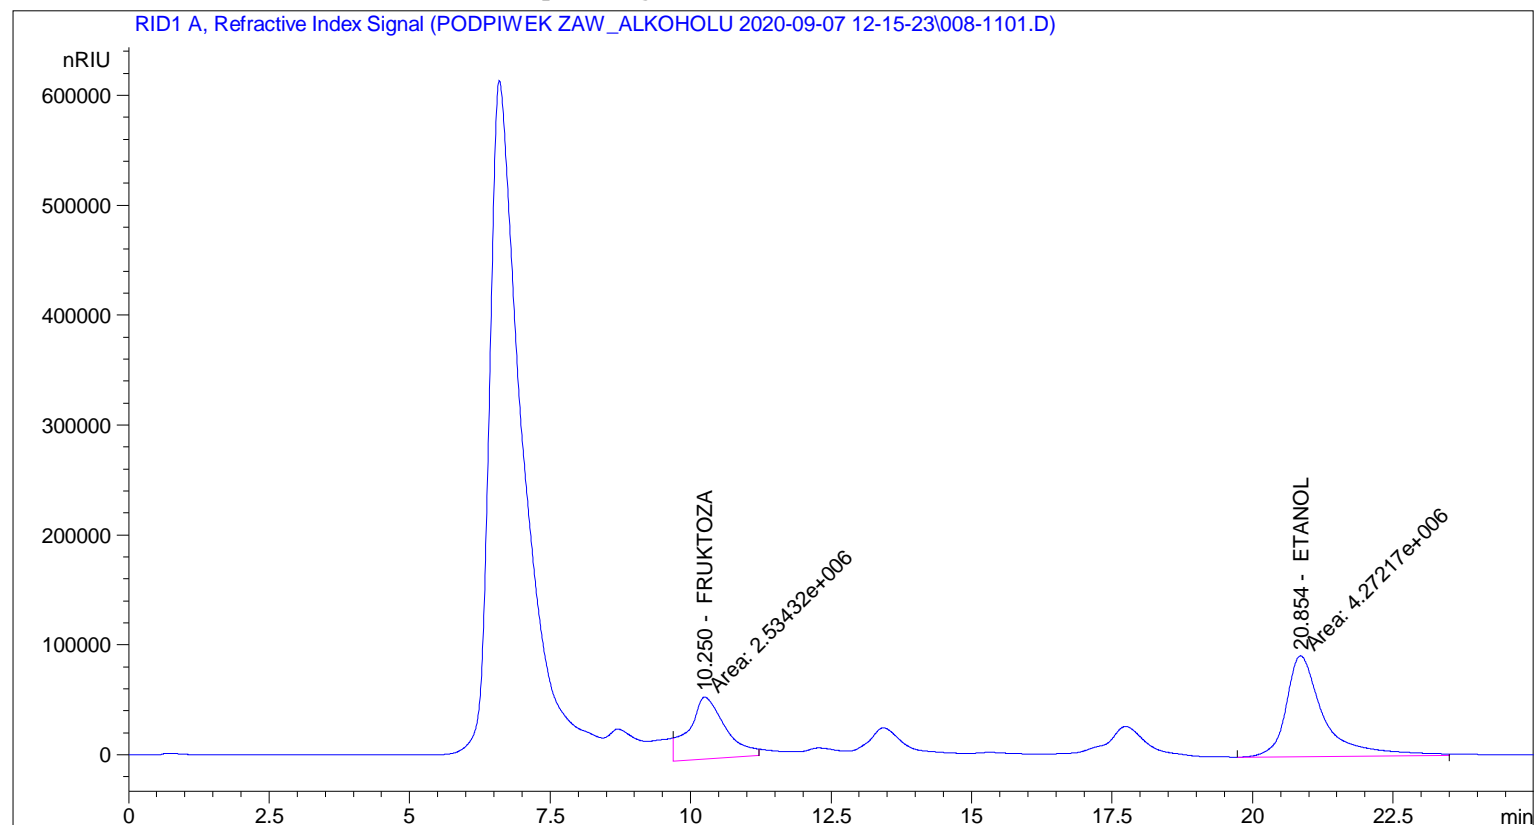

External Standard Report (Sample Amount is 0!)

```

Sorted By      :      Signal
Calib. Data Modified :      9/8/2020 11:48:18 AM
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
  
```

Signal 1: RID1 A, Refractive Index Signal

RetTime [min]	Type	Area [nRIU*s]	Amt/Area	Amount [%]	Grp	Name
7.849	-	-	-	-	-	MALTOZA
9.470	-	-	-	-	-	GLUKOZA
10.250	MM	2.53432e6	9.25410e-8	2.34528e-1	-	FRUKTOZA
20.854	MF	4.27216e6	2.72331e-7	1.16344	-	ETANOL

Totals : 1.39797

Sample Name: 8

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====

*** End of Report ***